

Fig. 1

00000000000000000000000000000000

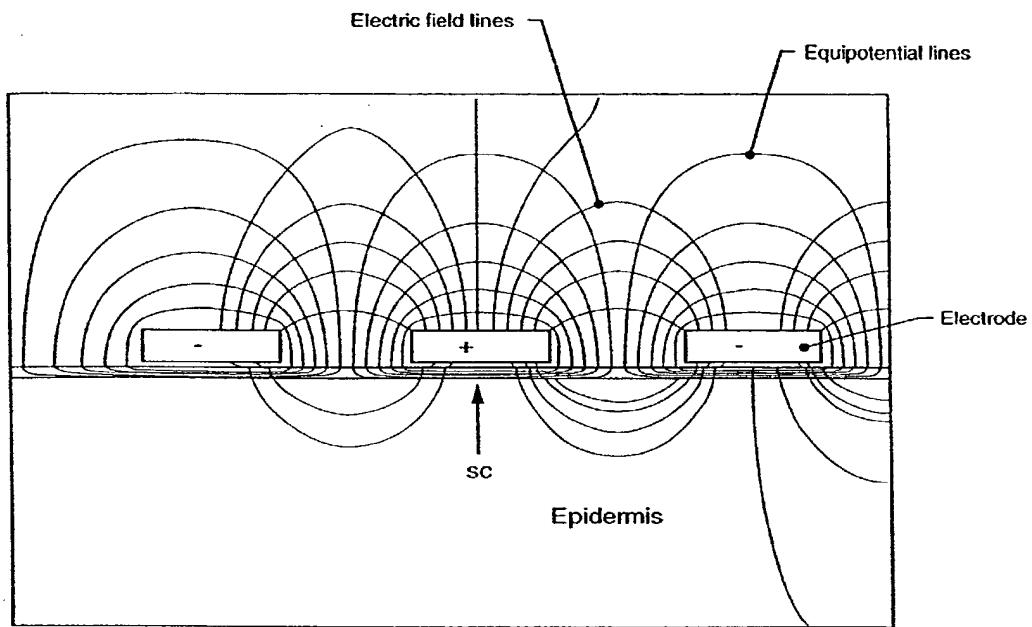


Fig. 2

FIELD STRENGTH BELOW AN ELECTRODE BEFORE BREAKDOWN OF THE S.C.

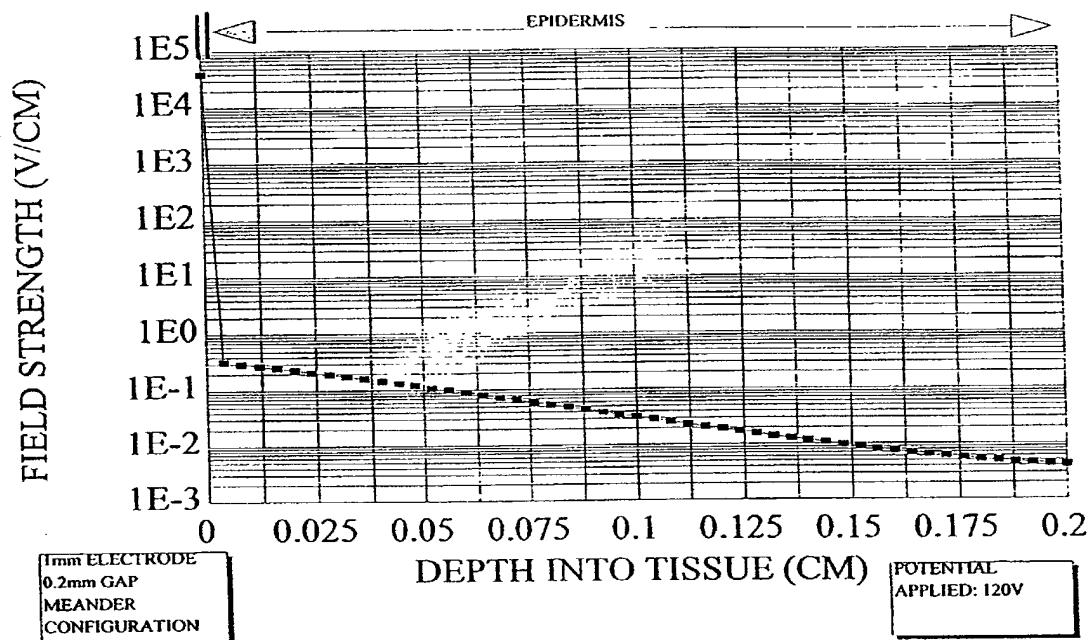


Fig. 3A

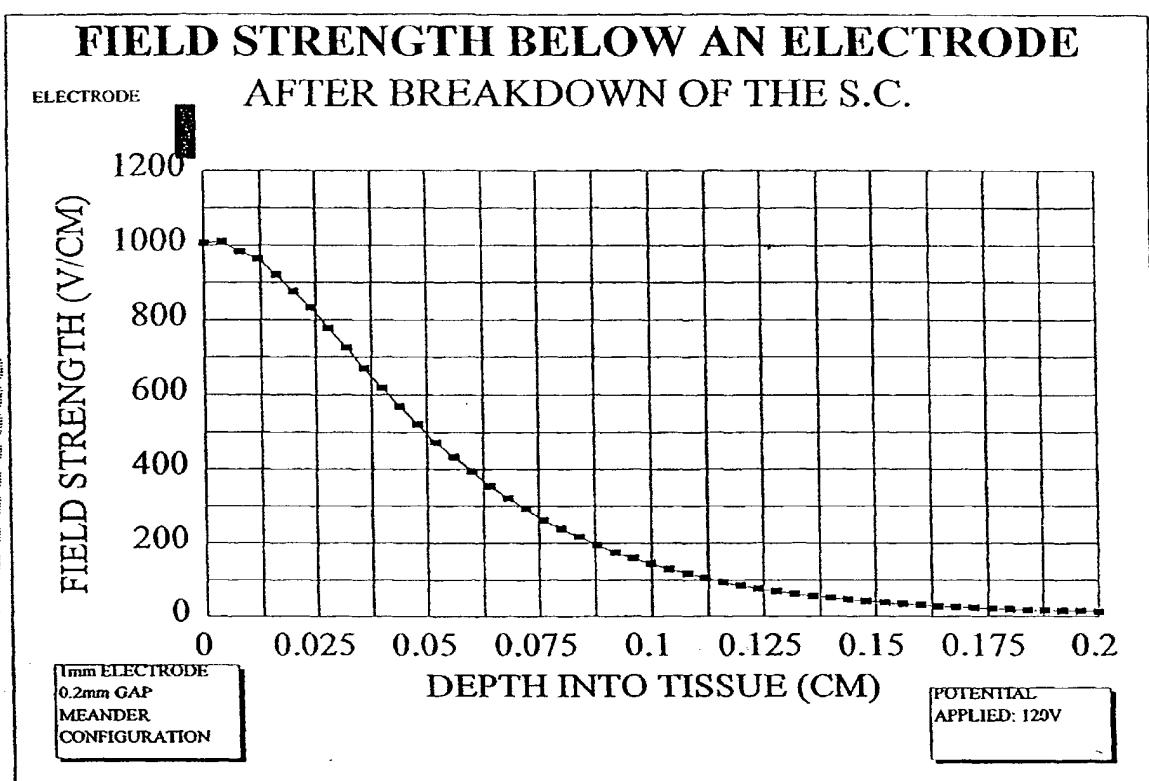


Fig. 3B

Field Across Tissue

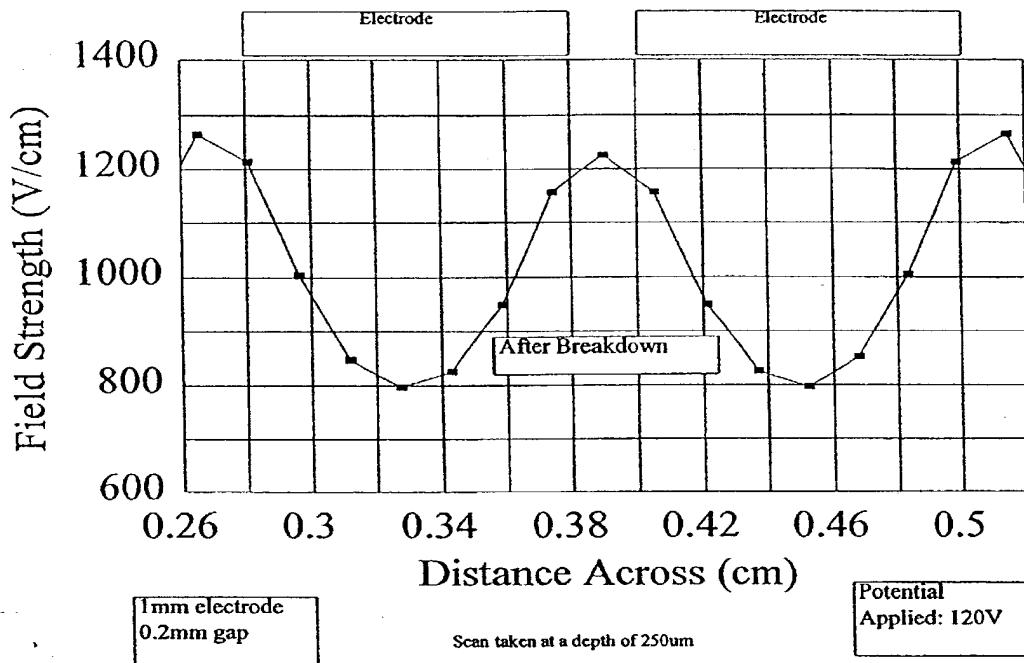


Fig. 4A

Field Across Tissue

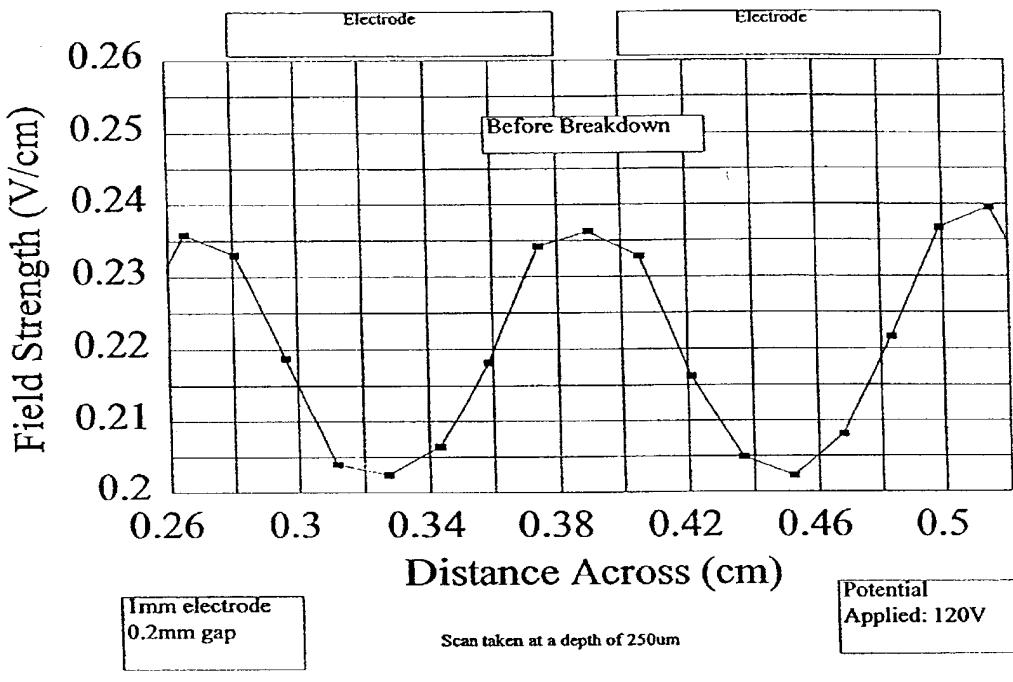


Fig. 4B

FIGURE 5A FIGURE 5B

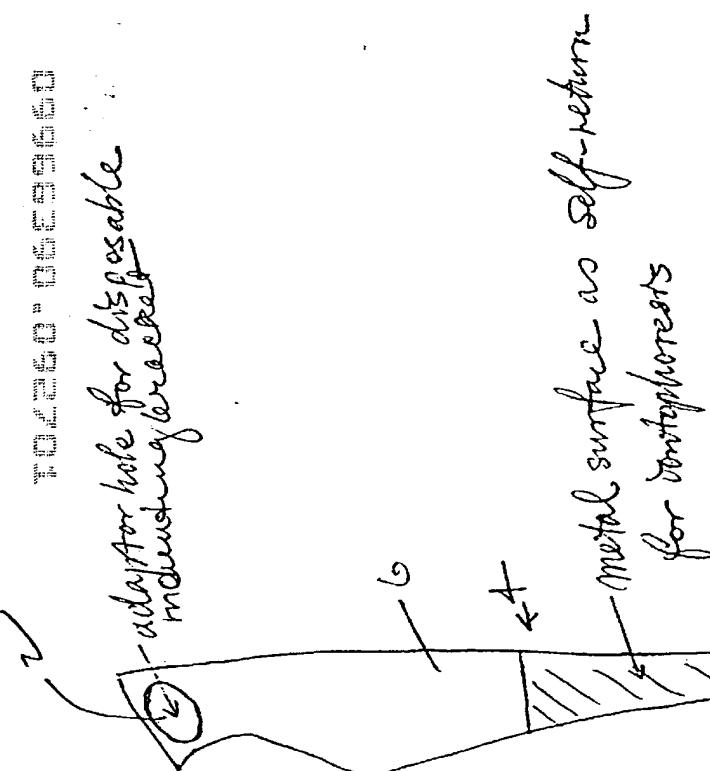


FIGURE 5A

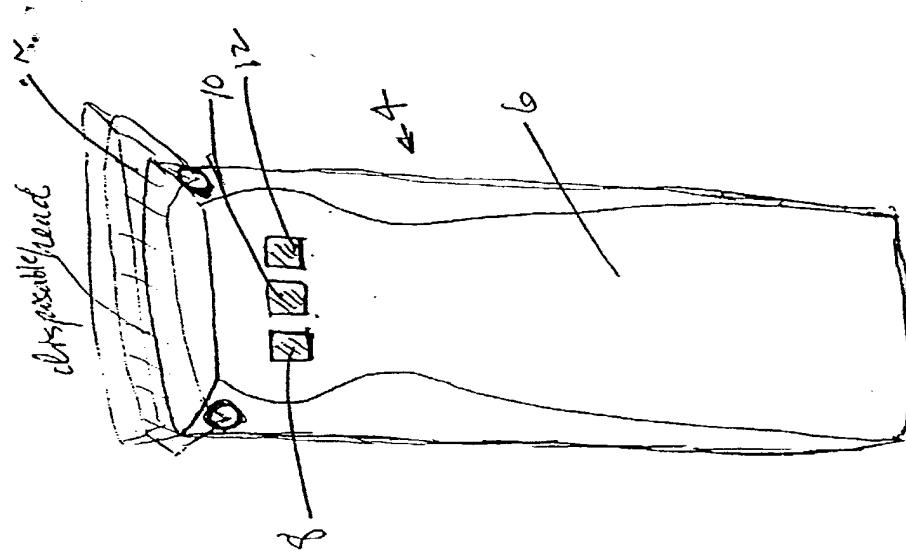


FIGURE 5B

Battery-powered hand held pulser
FIGURES 5A-B

卷之三



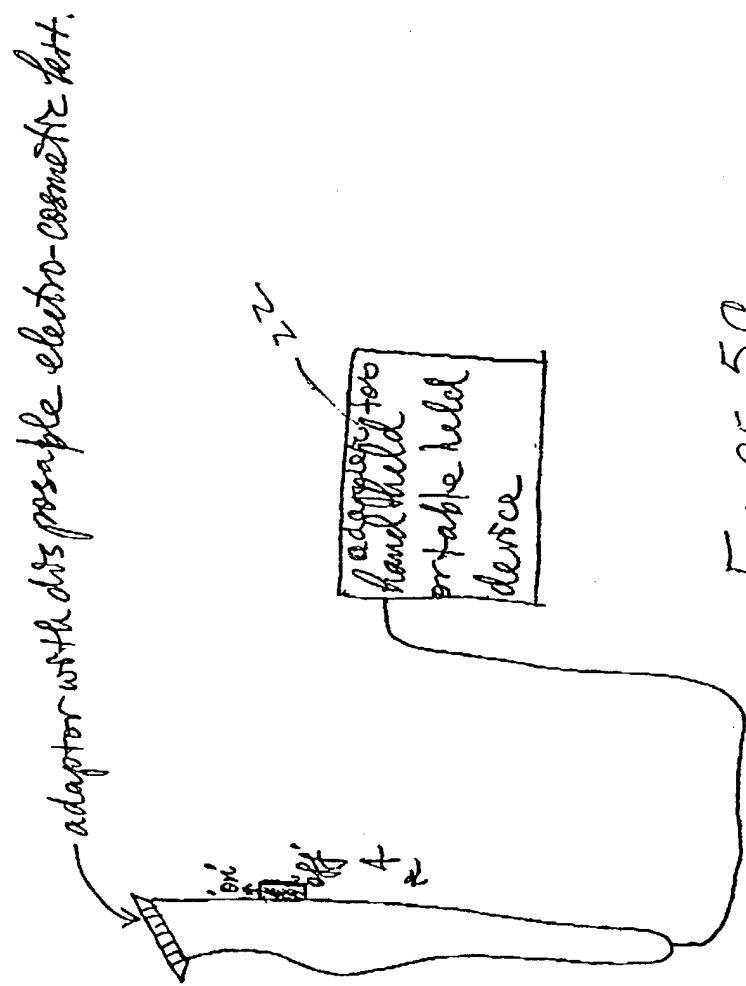


FIGURE 5C

Square type:

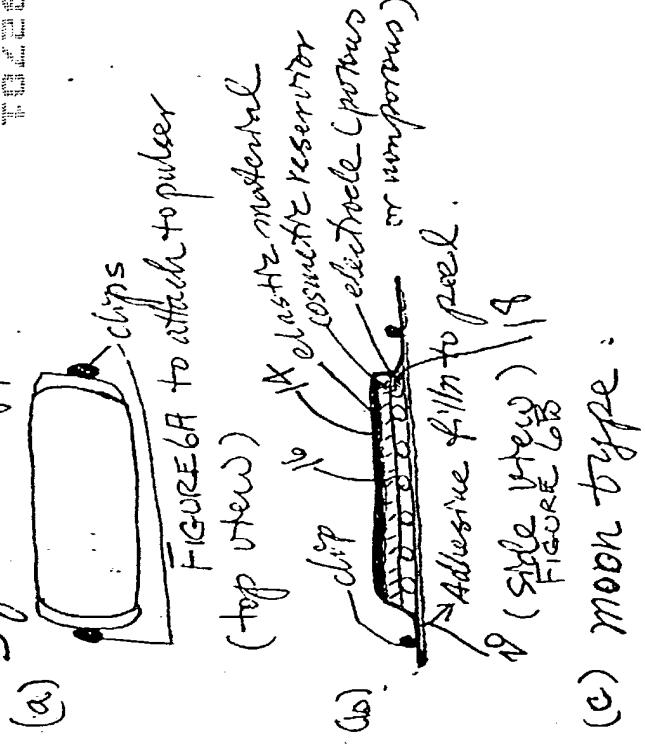

Moon type:

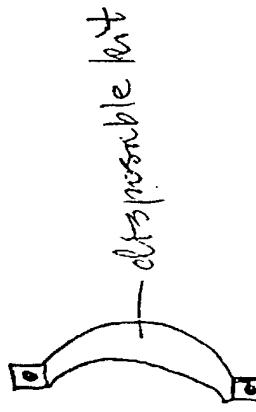

Moon type

FIGURE 6D
(top view)

FIGURE 6E
with cosmetic prep.


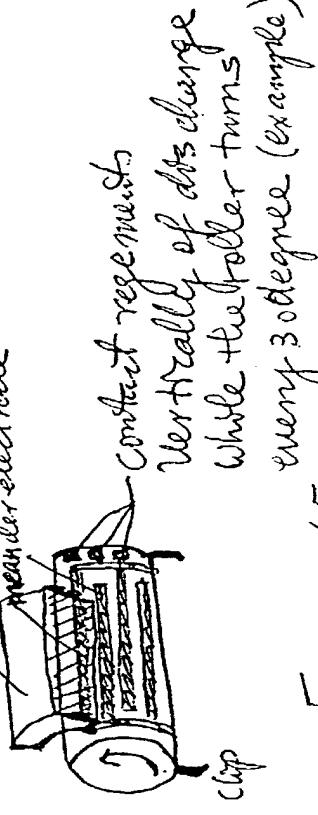


FIGURE 6E

FIGURES 6A-E
Different Configurations of disposable mounting bracket
size can be small or large

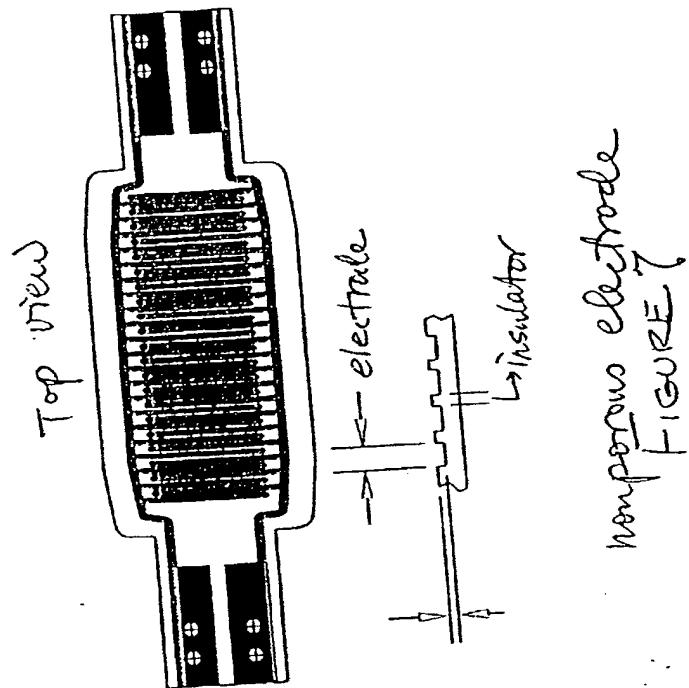

porous electrode
FIGURE 7